
Mehdi Moini

List of Publications by Year in descending order

Source: https://exaly.com/author-pdf/4153891/publications.pdf Version: 2024-02-01

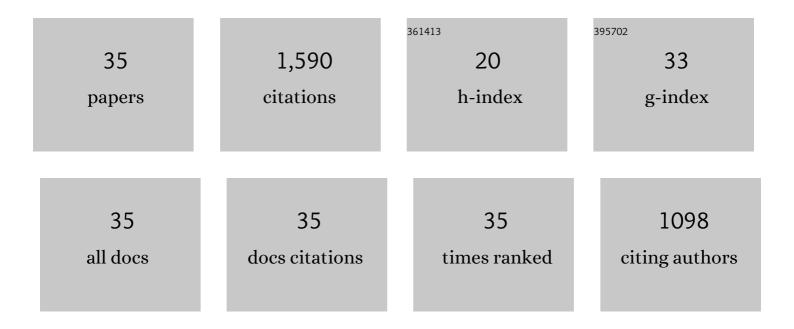

Менрі Моімі

#	Article	IF	CITATIONS
1	Analysis of ballpoint pen inks directly from paper using capillary electrophoresis. Forensic Chemistry, 2019, 13, 100145.	2.8	4
2	A comparison between DART-MS and DSA-MS in the forensic analysis of writing inks. Forensic Science International, 2018, 289, 27-32.	2.2	21
3	Buyid Silk and the Tale of Bibi Shahrbanu: Identification of Biomarkers of Artificial Aging (Forgery) of Silk. Analytical Chemistry, 2017, 89, 10158-10161.	6.5	7
4	Direct sample analysis-mass spectrometry vs separation mass spectrometry techniques for the analysis of writing inks. Forensic Chemistry, 2016, 1, 78-85.	2.8	12
5	Portable, Battery Operated Capillary Electrophoresis with Optical Isomer Resolution Integrated with Ionization Source for Mass Spectrometry. Journal of the American Society for Mass Spectrometry, 2016, 27, 388-393.	2.8	13
6	Dating Silk By Capillary Electrophoresis Mass Spectrometry. Analytical Chemistry, 2011, 83, 7577-7581.	6.5	47
7	Simplifying CEâ	6.5	290
8	Capillary Electrophoresis–Electrospray Ionization Mass Spectrometry of Amino Acids, Peptides, and Proteins. , 2004, 276, 253-290.		17
9	Application of capillary electrophoresis/ electrospray ionization-mass spectrometry to subcellular proteomics ofEscherichia coli ribosomal proteins. Electrophoresis, 2004, 25, 1981-1987.	2.4	50
10	Analysis of Underivatized Amino Acids and Theird/l-Enantiomers by Sheathless Capillary Electrophoresis/Electrospray Ionization-Mass Spectrometry. Analytical Chemistry, 2003, 75, 1508-1513.	6.5	83
11	CE/Electrospray Ionization-MS Analysis of Underivatized d/I-Amino Acids and Several Small Neurotransmitters at Attomole Levels through the Use of 18-Crown-6-tetracarboxylic Acid as a Complexation Reagent/Background Electrolyte. Analytical Chemistry, 2003, 75, 6282-6287.	6.5	82
12	Analysis of Carbonic Anhydrase in Human Red Blood Cells Using Capillary Electrophoresis/Electrospray Ionization-Mass Spectrometry. Analytical Chemistry, 2002, 74, 3772-3776.	6.5	50
13	Capillary electrophoresis mass spectrometry and its application to the analysis of biological mixtures. Analytical and Bioanalytical Chemistry, 2002, 373, 466-480.	3.7	131
14	Design and Performance of a Universal Sheathless Capillary Electrophoresis to Mass Spectrometry Interface Using a Split-Flow Technique. Analytical Chemistry, 2001, 73, 3497-3501.	6.5	67
15	Control of Electrochemical Reactions at the Capillary Electrophoresis Outlet/Electrospray Emitter Electrode under CE/ESI-MS through the Application of Redox Buffers. Analytical Chemistry, 2001, 73, 240-246.	6.5	54
16	Analysis of underivatized amino acid mixtures using high performance liquid chromatography/dual oscillating nebulizer atmospheric pressure microwave induced plasma ionization-mass spectrometry. Journal of the American Society for Mass Spectrometry, 2001, 12, 117-122.	2.8	41
17	Development of Multi-ESI-Sprayer, Multi-Atmospheric-Pressure-inlet Mass Spectrometry and Its Application to Accurate Mass Measurement Using Time-of-Flight Mass Spectrometry. Analytical Chemistry, 2000, 72, 20-24.	6.5	54
18	Separation and detection of the α- and β-chains of hemoglobin of a single intact red blood cell using capillary electrophoresis/electrospray ionization time-of-flight mass spectrometry. Journal of the American Society for Mass Spectrometry, 1999, 10, 184-186.	2.8	30

Mehdi Moini

#	Article	IF	CITATIONS
19	Hydroquinone as a Buffer Additive for Suppression of Bubbles Formed by Electrochemical Oxidation of the CE Buffer at the Outlet Electrode in Capillary Electrophoresis/Electrospray Ionization-Mass Spectrometry. Analytical Chemistry, 1999, 71, 1658-1661.	6.5	67
20	Pressure-assisted and pressure-programmed capillary electrophoresis/electrospray ionization time of flight - mass spectrometry for the analysis of peptide mixtures. Electrophoresis, 1998, 19, 2200-2206.	2.4	26
21	Capillary electrophoresis/electrospray ionization high mass accuracy time-of-flight mass spectrometry for protein identification using peptide mapping. , 1998, 12, 864-870.		33
22	Atmospheric pressure microwave induced plasma ionization source for molecular mass spectrometry. Journal of the American Society for Mass Spectrometry, 1998, 9, 42-49.	2.8	7
23	Sodium trifluoroacetate as a tune/calibration compound for positive- and negative-ion electrospray ionization mass spectrometry in the mass range of 100–4000 Da. Journal of the American Society for Mass Spectrometry, 1998, 9, 977-980.	2.8	92
24	Analysis of peptides, proteins, protein digests, and whole human blood by capillary electrophoresis/electrospray ionization-mass spectrometry using an in-capillary electrode sheathless interface. Journal of the American Society for Mass Spectrometry, 1998, 9, 1081-1088.	2.8	60
25	A novel sheathless interface for capillary electrophoresis/electrospray ionization mass spectrometry using an in-capillary electrode. Journal of the American Society for Mass Spectrometry, 1997, 8, 561-564.	2.8	88
26	Selective Detection of Selenium in Water Utilizing Chemical Reaction Interface Mass Spectrometryâ€. Journal of Mass Spectrometry, 1997, 32, 420-424.	1.6	9
27	Rapid Derivatization and Gas Chromatography/Mass Spectrometry Analysis of Dipeptides in Aqueous Solution. Rapid Communications in Mass Spectrometry, 1997, 11, 349-352.	1.5	9
28	Design and performance of a high resolution electrospray ion source for a magnetic sector mass spectrometer with a heated capillary inlet. Journal of the American Society for Mass Spectrometry, 1995, 6, 1256-1261.	2.8	9
29	Conversion of the Finniganâ€MAT TSQâ€70 thermospray ionization interface to an electrospray ionization interface. Review of Scientific Instruments, 1994, 65, 591-596.	1.3	12
30	Ultramark 1621 as a calibration/reference compound for mass spectrometry. II. Positive- and negative-ion electrospray ionization. Rapid Communications in Mass Spectrometry, 1994, 8, 711-714.	1.5	42
31	Characterization of fluorinated ethylchloroformate derivatives of protein amino acids using positive and negative chemical ionization gas chromatography/mass spectrometry. Biological Mass Spectrometry, 1994, 23, 277-282.	0.5	18
32	Fomblin as a reference compound for negative ion fast atom bombardment high-resolution mass spectrometry in the mass range of 180-3000 u. Biological Mass Spectrometry, 1993, 22, 170-175.	0.5	2
33	Ultramark 1621 as a reference compound for positive and negative ion fast-atom bombardment high-resolution mass spectrometry. Journal of the American Society for Mass Spectrometry, 1992, 3, 842-846.	2.8	25
34	Isomerization of linear C3H3+ in its reaction with acetylene, and collisional stabilization of the [C5H5+]* collision complex in a quadrupole ion trap mass spectrometer. Journal of the American Society for Mass Spectrometry, 1992, 3, 631-636.	2.8	19
35	Selective detection and characterization of chlorine- and bromine-containing compounds in complex mixtures using microwave-induced plasma/chemical reaction interface mass spectrometry. Biological Mass Spectrometry, 1992, 21, 693-699.	0.5	19